

Calibrating Unit

New Standard Solution Report

Equipment: Alcotest 7110 MKIII-C	Serial No.:	ARXC-0091
Location: CEDAR GROVE POLICE		
Calibration File No.: 00870	Calib. Date: 05/13/2022	Calib. No.: 00035
Certification File No.: 00871	Cert. Date: 05/13/2022	Cert. No.: 00030
Linearity File No.: 00872	Lin. Date: 05/13/2022	Lin. No.: 00030
Solution File No.: 00874	Soln. Date: 06/09/2022	Soln. No.: 00225
Sequential File No.: 00874	File Date: 06/09/2022	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDZH-0063
Control Solution %: 0.100%		Expires: 05/04/2023
Solution Control Lot: 21150		Bottle No.: 0549

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:09D		
Control 1 EC	0.099%	15:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	15:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:10D		
Control 2 EC	0.099%	15:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:11D		
Control 3 EC	0.099%	15:12D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HOYT

First Name: NICOLE

MI: -

Signature: _____

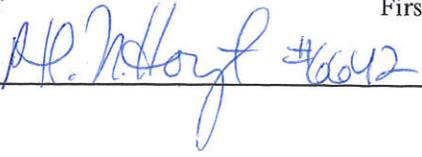

Badge No.: 6642

Date: 06/09/2022