


STATE OF NEW JERSEY
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
BREATH TESTING INSTRUMENTATION SERVICE REPORT

1. Department: Cedar Grove Police Department 525 Pompton Avenue Cedar Grove, NJ 07009	2. Contact: Lt. Frank Pumphrey 3. Phone Number: 973-239-4100	4. Date: 02/07/2022 5. County: Essex
6. Alcotest Instrument Serial Number: <p style="text-align: center;">N/A</p>	7. Simulator Component Serial Number: <p style="text-align: center;">DDZH-0064</p>	8. Temperature Probe Component Serial Number: <p style="text-align: center;">DDXK P2-321</p>

9. Reason for Service:
Arrived at the department to conduct a simulator probe change.

10. Comments:
I observed, the simulator serial number DDZH-0064 was not turning on. I tried multiple electrical outlets obtaining the same results. The simulator was taken out of service and will be sent to Draeger for further evaluation.

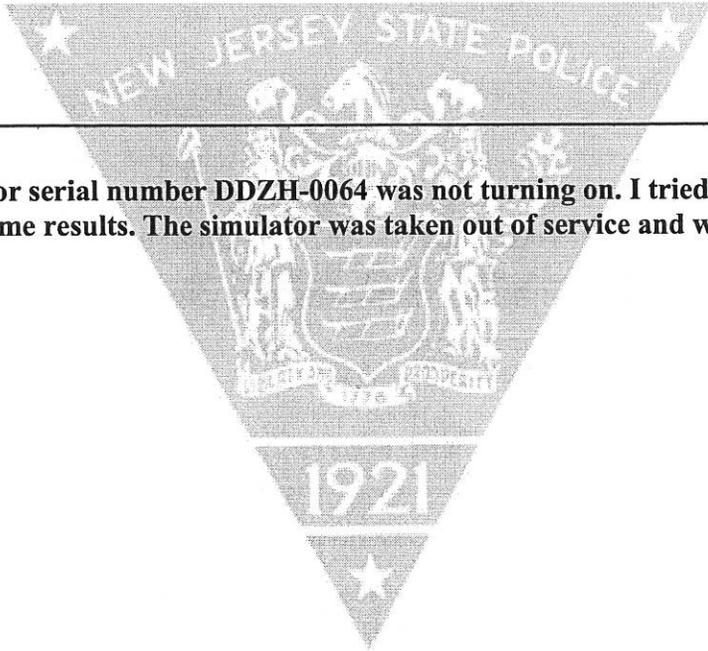

Last Known Sequential File #: N/A

11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
12. The above Instrument/Component is placed out of service pending further evaluation.
13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

Tpr. II Francisco A. Hurtado #7635
Name & Badge Number (Print)

Tpr. II Francisco A. Hurtado #7635 2-7-22
Signature Date