


STATE OF NEW JERSEY  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
**BREATH TESTING INSTRUMENTATION SERVICE REPORT**

1. Department: <b>CEDAR GROVE POLICE DEPARTMENT</b> <b>525 POMPTON AVE.</b> <b>CEDAR GROVE NJ 07009</b>		2. Contact: <b>SGT. F. PUMPHREY</b>	4. Date: <b>04-24-2013</b>
		3. Phone Number: <b>973-239-4143</b>	5. County: <b>ESSEX</b>
6. Alcotest Instrument Serial Number: <p style="text-align: center;"><b>ARXC-0091</b></p>	7. Simulator Component Serial Number: <p style="text-align: center;"><b>N/A</b></p>	8. Temperature Probe Component Serial Number: <p style="text-align: center;"><b>N/A</b></p>	

9. Reason for Service:  
**FUEL CELL REPLACEMENT**

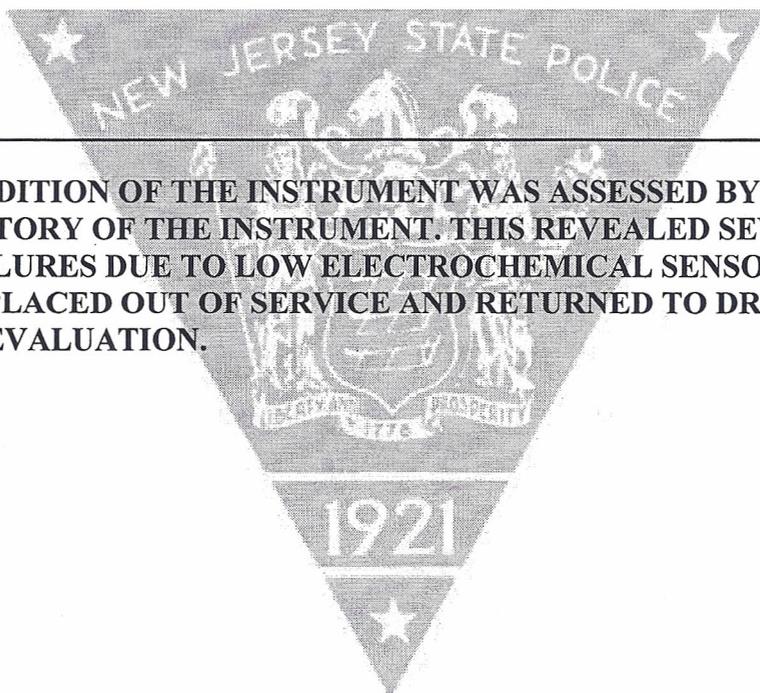

10. Comments:  
**OPERATIONAL CONDITION OF THE INSTRUMENT WAS ASSESSED BY REVIEWING THE PERFORMANCE HISTORY OF THE INSTRUMENT. THIS REVEALED SEVERAL REPEATED CONTROL TEST FAILURES DUE TO LOW ELECTROCHEMICAL SENSOR (EC) RESULTS. INSTRUMENT WAS PLACED OUT OF SERVICE AND RETURNED TO DRAEGER SAFETY DIAGNOSTICS FOR EVALUATION.**

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."


**TPR I. M. ARROYO #6291**  
 Name & Badge Number (Print)

*Ipc I. M. Arroyo* 6291 4/24/13  
 Signature Date

STATE OF NEW JERSEY  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
**BREATH TESTING INSTRUMENTATION SERVICE REPORT**

1. Department: <b>CEDAR GROVE POLICE DEPART. 525 POMPTON AVE. CEDAR GROVE NJ 07009</b>		2. Contact: <b>SGT. F. PUMPHREY</b>	4. Date: <b>05-08-2013</b>
		3. Phone Number:	5. County: <b>ESSEX COUNTY</b>
6. Alcotest Instrument Serial Number: <p style="text-align: center;"><b>ARXC-0091</b></p>	7. Simulator Component Serial Number: <p style="text-align: center;"><b>N/A</b></p>	8. Temperature Probe Component Serial Number: <p style="text-align: center;"><b>N/A</b></p>	

9. Reason for Service:  
**PLACED BACK INTO SERVICE**

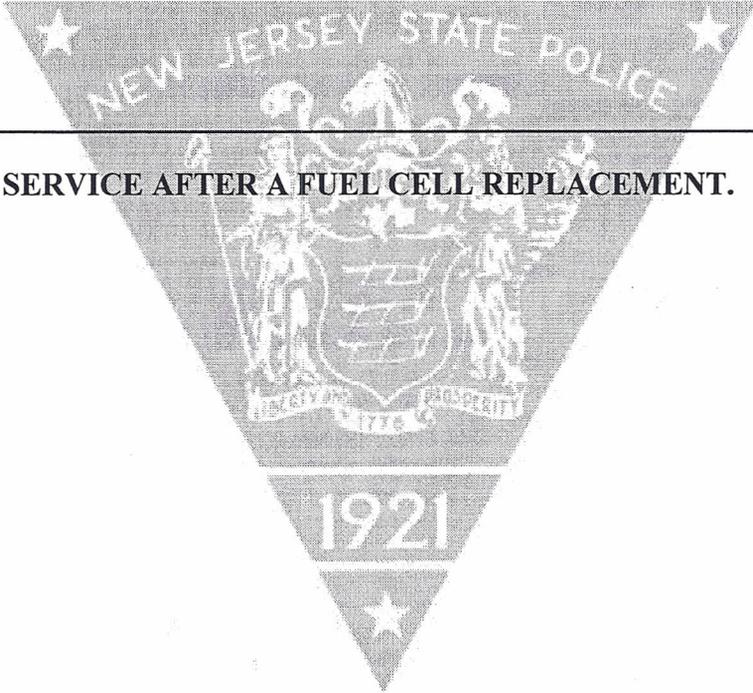

10. Comments:  
**PLACED BACK INTO SERVICE AFTER A FUEL CELL REPLACEMENT.**

- 11. The above Instrument/Component has been found to be in satisfactory working condition; no further action required.
- 12. The above Instrument/Component is placed out of service pending further evaluation.
- 13. The above Instrument/Component is placed back in service.

"I have been certified by the Attorney General as a Breath Test Coordinator/Instructor pursuant to N.J.A.C. 13:51, et. seq. In my official capacity as a Breath Test Coordinator/Instructor I perform inspections of evidential breath test devices and related components of evidential breath test systems. I have inspected the evidential breath test device listed on this report in my official capacity. The results of my inspection are recorded on this form. I certify that the forgoing statements made by me are true and accurate to the best of my knowledge. I am aware that if any of the forgoing statements made by me are willingly false, I am subject to punishment."

**TPR I. M. ARROYO #6291**  
 Name & Badge Number (Print)

*I. M. Arroyo*  
 Signature **6291 5/8/2013**  
 Date

# Packing Slip

Customer no    Order No    Order date  
 150077315    10622031    05/01/2013

Packing slip no.    Ship date  
 80770715    05/01/2013

Please reference on inquiries

ship to  
 150077315  
 TOWNSHIP OF CEDAR GROVE P.D.  
 ATTN: FRANCIS M. PUMPHREY  
 525 POMPTON AVE.  
 CEDAR GROVE, NJ 07009  
 USA

bill to

Your Purchase Order Number

7110: ARXC-0091  
 Any questions? Please contact:  
 AMANDA DILLEY

Customer  
 TOWNSHIP OF CEDAR GROVE P.D.  
 ATTN: FRANCIS M. PUMPHREY  
 525 POMPTON AVE.  
 CEDAR GROVE, NJ 07009  
 USA

Your sales person

Don Pouliot  
 Phone: 973-398-3228

Delivery terms  
 FA  
 FREIGHT ALLOWED

Item#	sh. Quant.	Part no. Description			
		Ship via: Fed Ex Saver			
		NOTE: All claims for shortages/defects must be reported within 10 Business days after receipt of order. All returns must have our RMA# clearly marked on the box. Please call Customer Service at 866-385-5900.			
0010	1 EA	MPCAL71 CALIBRATION CHARGE - 7110/9510 Ordered / Back ordered : 0 / 0 EA			
0020	1 EA	6808455 SENSOR : FUEL CELL Ordered / Back ordered : 0 / 0 EA			

**Draeger Safety Diagnostics Inc.**  
 Accounting Address:  
 101 Technology Drive  
 Pittsburgh, PA 15275  
 Tel: (412) 788-5537  
 Fax: (412) 788-5598

**Remit Wire Transfers To:**  
 Citizens Bank  
 Acct. # 6209426615  
 Acct. Name: Draeger Safety Diagnostics Inc.  
 Transit Number: 036076150  
 Federal ID Number: 84-1600159

**REMIT TO:**  
 Draeger Safety Diagnostics Inc.  
 P.O. Box 200337  
 Pittsburgh, PA 15251-0337

# Packing Slip

Customer no    Order No    Order date  
150077315    10622031    05/01/2013

Packing slip no.    Ship date  
80770715    05/01/2013

Please reference on inquiries

Page    2 / 2

Item#	sh. Quant.	Part no. Description			
0030	1 EA	6808486 PLATES, 7110--9510 Ordered / Back ordered : 0 / 0 EA			
0040	0.5 H	MPLABOR LABOR CHARGE Ordered / Back ordered : 0.0 / 0.0 H			

# RETURN AND REPAIR FORM



## Customer Information

B: \_\_\_\_\_

S: \_\_\_\_\_

Company Name: Cedar Grove P.D., Cedar Grove, NJ

Date Received: 04/29/13

Date given to service: 04/29/13

Carrier:  FedEx  UPS  USPS Shipping Method:  GRD  3DAY  2DAY  
 NDA-PRI  NDA-STD

Product:  6510  6810  
 7110  8610  
 7510  DT5000  
 7410 Upper-half  9510  
 7410 Whole

Serial Number: AR XC-0091

Printer Serial#: AR

Sim Serial#: DD

Probe Serial#: DD

Warranty Expires: December 2013

Description:  A  B  Plus  Demo  Screener  Trade In

## Accessories

110V A/C Adapter  Regulator  Printer Ribbon  Printer Paper  
 Mouthpieces  9510 Stylus  9510 Top Cover  Carrying Case  
 Dry Gas  Other (please specify) \_\_\_\_\_

## Repair Information:

Test#: \_\_\_\_\_

Part Number	Description	Qty	Total Cost
MP Cal 71	Calibration	1	NC/W
6808455	Fuel Cell	1	NC/W
6808486	Spacer Plate	2	NC/W
MP Labor	Labor	.5	NC/W

Repair Notes: Replaced defective fuel cell and spacer plate.

Fuel Cell AREA-3285

CAL W/QC AND OPS CHECK

Service Technician BC

Date: 05/01/13